

DSA
Delta TRAC

A Division of: Delta Sales Associates Inc., 8171 Main Street, Buffalo, NY 14221 • Ph: (716) 631-8103 • Fx: (716) 631-8108

STATEMENT OF CALIBRATION

Certificate #: LRW090814-01



Calibration Certificate #: 1569.01

Company: Metalife Industries, Inc.	Reference PO #: PUR495
Address: 141 Mong Way, Reno, PA 16343	

Instrument: Fischer Couloscope CMS	Serial #: 110007164	Condition: In Tolerance
---	----------------------------	--------------------------------

The above instrument has been inspected and calibrated and was found to be in operable working condition. This determination was made using a N.I.S.T. traceable thickness standard and following ISO/IEC 17025:2005 and ANSI/NC SL Z540.1-1994 accredited procedures. The results below relate only to the instrument calibrated.

Date Calibrated: 09/08/14	Calibration Due Date: 09/30/15
Calibration Procedure Used: Coulometric	Procedure #: 1028954

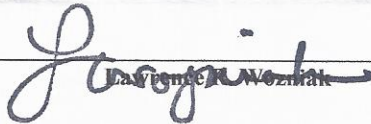
N.I.S.T. Traceable Standards Certification:

Standard	S/N	Value	"As Found"	"As Left"	% Unc*
Ni/Fe	Ni-55036	0.516 mils	0.500 mils	0.503 mils	13.83%

*This value represents an expanded uncertainty expressed at the 95% C.L. using a coverage factor of k=2.

Temperature: 70.4°F	Humidity: 42.0% RH
----------------------------	---------------------------

Field:	Lab: X
---------------	---------------

Certified By: 

Date of Issue: 09/08/14

PLEASE NOTE: Conditions affecting the calibration, such as standard wear, corrosion, electrolyte shelf life, electronic drift, etc., may affect the performance of this instrument during the recommended calibration interval, such that it may drift out of tolerance. It is recommended that the actual working calibration of this instrument be verified by the user on a regular basis according to manufacturer's specifications.

The liability of Delta TRAC, Division of Delta Sales Associates, Inc., is limited to the cost of the certification of this instrument. Delta TRAC is not responsible for any monetary, incidental or consequential damages resulting from the use of this instrument. This certificate shall not be reproduced in full or part without the express written consent of Delta TRAC.